




Electromagnetic acoustic transducer S7694

DATA SHEET

MAIN TECHNICAL SPECIFICATION


Transducer type:	straight-beam electromagnetic acoustic transducer with permanent magnet for generating and receiving shear waves with linear polarization	
Nominal frequency:	3 MHz ± 10%	
Effective aperture diameter:	18x12 mm	
Inspection range:	1 to 200 mm (when using A1270 EMAT)	
Lift-off/through-coating thickness:	up to 4 mm (for inspection range up to 50 mm)	
Maximal excitation pulse voltage:	600 V	
Direct current resistance of signal inductor:	7 ± 2 Ohm	
Operating temperature rang:	-30 to +60 °C	
Overall dimensions:	40x56 mm	
Type of socket:	LEMO ERN.00.250	
Weight:	215 g	

MEASUREMENT CONDITIONS AND EQUIPMENT


Reference excitation signal: unipolar square pulse with amplitude $400 \text{ V} \pm 40 \text{ V}$, pulse duration $200 \pm 13 \text{ ns}$ by 50% of the maximum voltage amplitude.
 Reference block: CO-2, steel 20, serial number 006 longitudinal wave velocity 5930 m/s, shear waves velocity 3247 m/s.
 Measured pulse: echo pulse from the backwall of reference block, depth 30 mm.
 Induced noise: white thermal noise with 2 mV effective amplitude, generated in inductor coil placed adjacent to the protector of the transducer.

MEASURED CHARACTERISTICS

Shape of the measured echo pulse

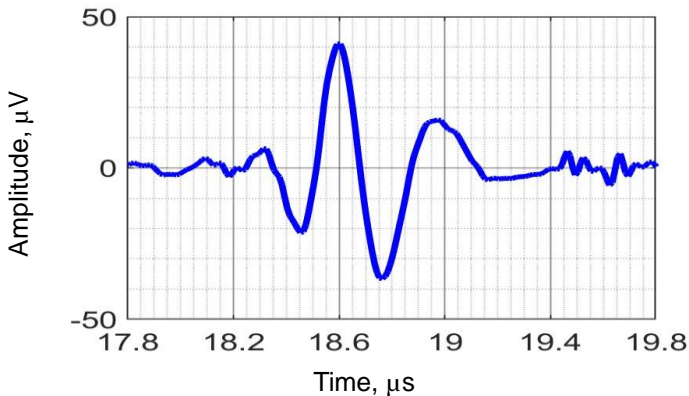


Amplitude frequency response

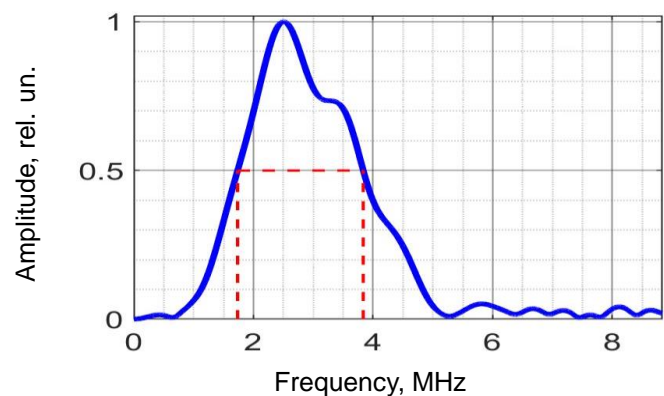

Echo pulse duration: **0.97 µs**
 Echo pulse amplitude A_e : **40.9 µV**
 Bandwidth II: **2.1 MHz**
 Relative bandwidth B_w : **75%**

Peak frequency f_p : **2.5 MHz**
 Lower cut-off frequency f_l : **1.7 MHz**
 Upper cut-off frequency f_u : **3.8 MHz**
 Centre frequency f_c : **2.8 MHz**

Reverberation noise curve (RNC)

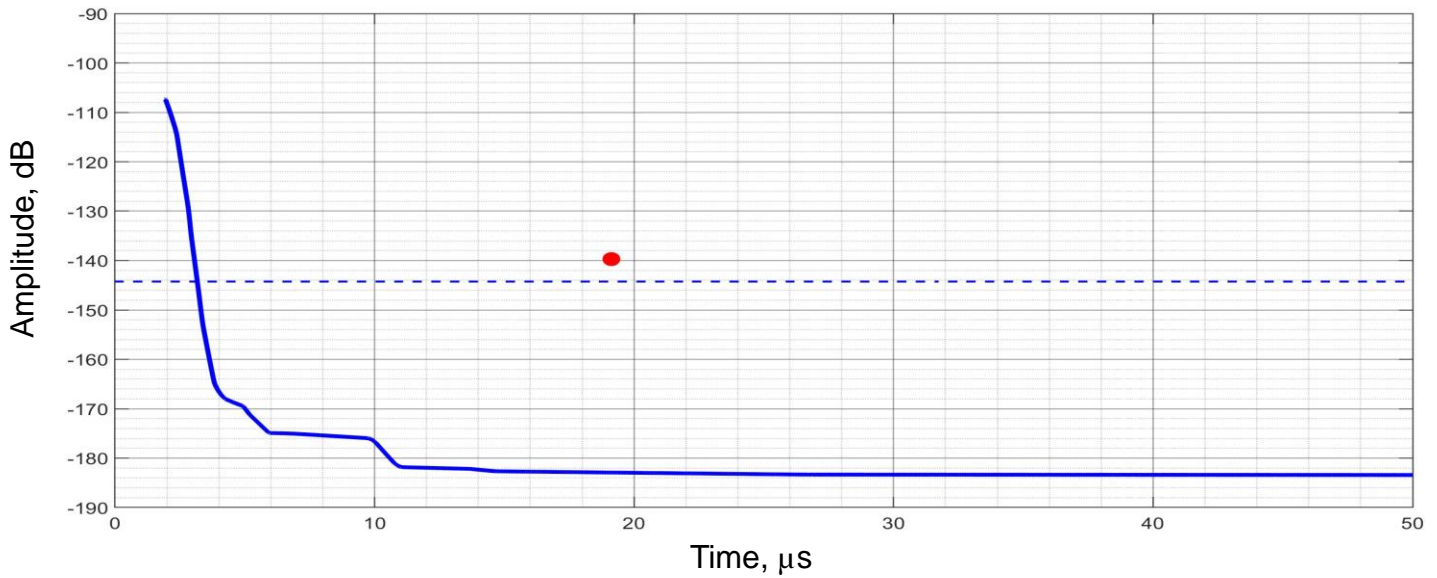

Signal-to-noise ratio between the backwall signal in the reference block and transducer self-noise:

43 dB


Signal-to-noise ratio between the backwall signal in the reference block and transducer self-noise in presence of electromagnetic noise:

5 dB

RNC level at 5 μs:

-170 dB

Autocorrelation function (ACF)

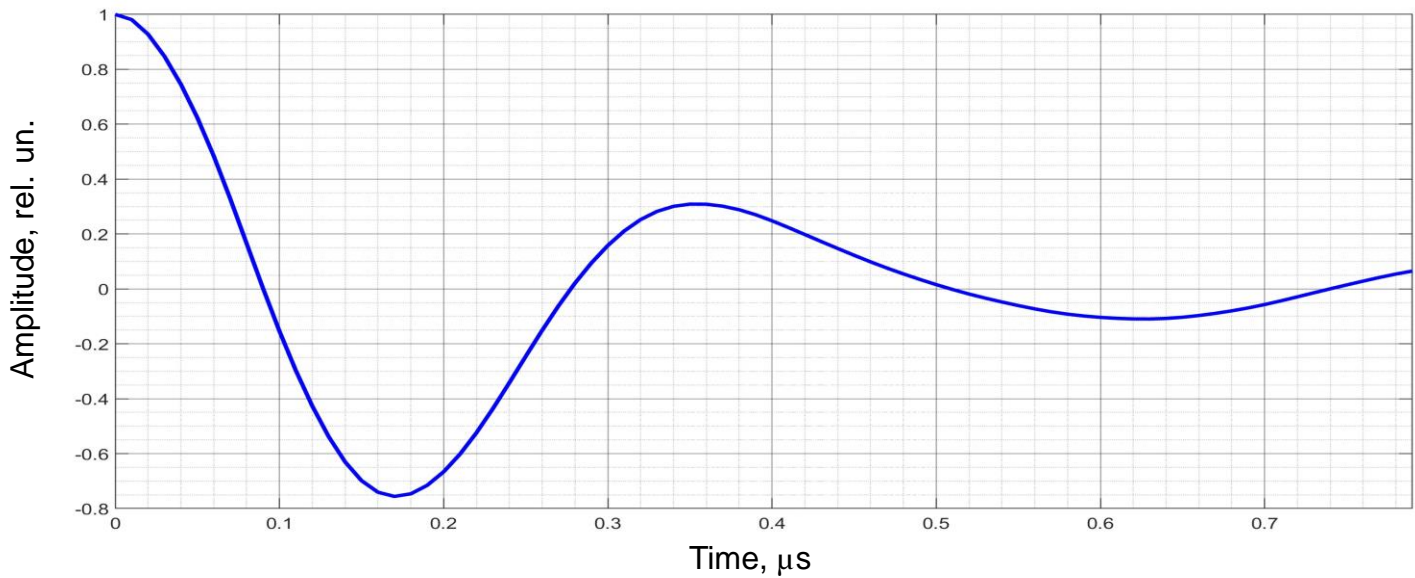

Amplitude of the first maximum of ACF:

0.31

Time position of the first maximum of ACF:

0.35 μs

Note:

The RNC is normalized by test excitation signal amplitude and given in logarithmic scale. Transducer RNC is indicated by the solid line. The dash line shows the amplitude of induced noise in sum with the RNC. The dot indicates the echo pulse amplitude received on the CO-2 reference block.